

Excellent Integrated System Limited

Stocking Distributor

Click to view price, real time Inventory, Delivery & Lifecycle Information:

[Infineon Technologies](#)

[BGX 50A E6327](#)

For any questions, you can email us directly:


sales@integrated-circuit.com




BGX50A...

Silicon Switching Diode Array

- Bridge configuration
- High-speed switching diode chip
- Pb-free (RoHS compliant) package¹⁾
- Qualified according AEC Q101

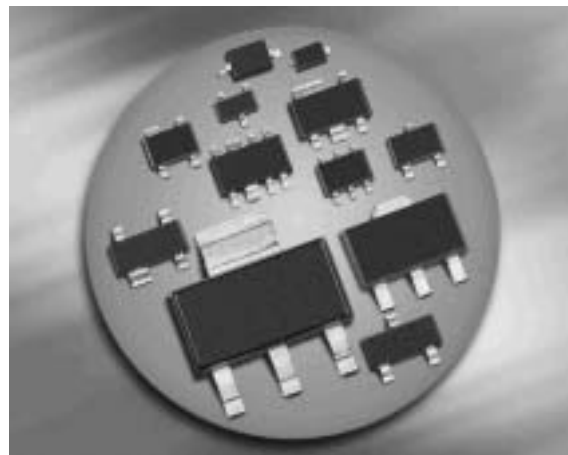

BGX50A



Type	Package	Configuration	Marking
BGX50A	SOT143	bridge	U1s

Maximum Ratings at $T_A = 25^\circ\text{C}$, unless otherwise specified

Parameter	Symbol	Value	Unit
Diode reverse voltage	V_R	50	V
Peak reverse voltage	V_{RM}	70	
Forward current	I_F	140	mA
Non-repetitive peak surge forward current	I_{FSM}	-	
Total power dissipation $T_S \leq 74^\circ\text{C}$	P_{tot}	210	mW
Junction temperature	T_j	150	$^\circ\text{C}$
Storage temperature	T_{stg}	-65 ... 150	

Thermal Resistance

Parameter	Symbol	Value	Unit
Junction - soldering point ²⁾ BGX50A	R_{thJS}	360	K/W

¹Pb-containing package may be available upon special request

²For calculation of R_{thJA} please refer to Application Note Thermal Resistance



BGX50A...


Electrical Characteristics at $T_A = 25^\circ\text{C}$, unless otherwise specified

Parameter	Symbol	Values			Unit
		min.	typ.	max.	
DC Characteristics					
Breakdown voltage	$V_{(BR)}$	-	-	-	
Reverse current	I_R				μA
$V_R = 50\text{ V}$		-	-	0.2	
$V_R = 50\text{ V}, T_A = 150^\circ\text{C}$		-	-	100	
Forward voltage	V_F	-	-	1.3	V
$I_F = 100\text{ mA}$					

AC Characteristics

Diode capacitance	C_T	-	-	1.5	pF
$V_R = 0\text{ V}, f = 1\text{ MHz}$					
Reverse recovery time	t_{rr}	-	-	6	ns
$I_F = 10\text{ mA}, I_R = 10\text{ mA}$, measured at $I_R = 1\text{ mA}$, $R_L = 100\ \Omega$					

Test circuit for reverse recovery time

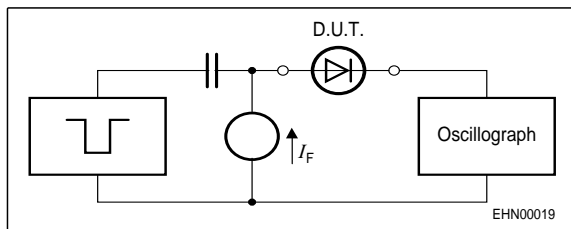

Pulse generator: $t_p = 100\text{ ns}$, $D = 0.05$, $t_r = 0.6\text{ ns}$,
 $R_i = 50\ \Omega$


Oscilloscope: $R = 50\ \Omega$, $t_r = 0.35\text{ ns}$, $C \leq 1\text{ pF}$



BGX50A...


Reverse current $I_R = f(T_A)$

$V_R =$ Parameter

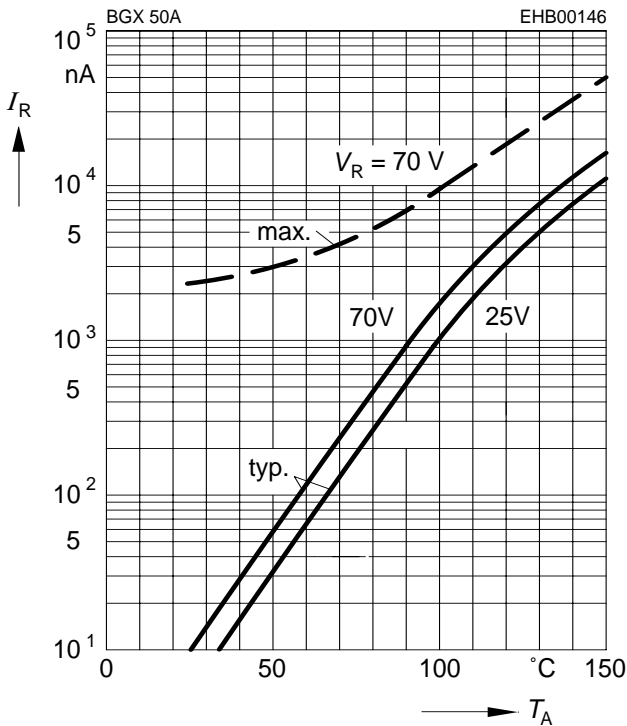


Forward Voltage $V_F = f(T_A)$

$I_F =$ Parameter

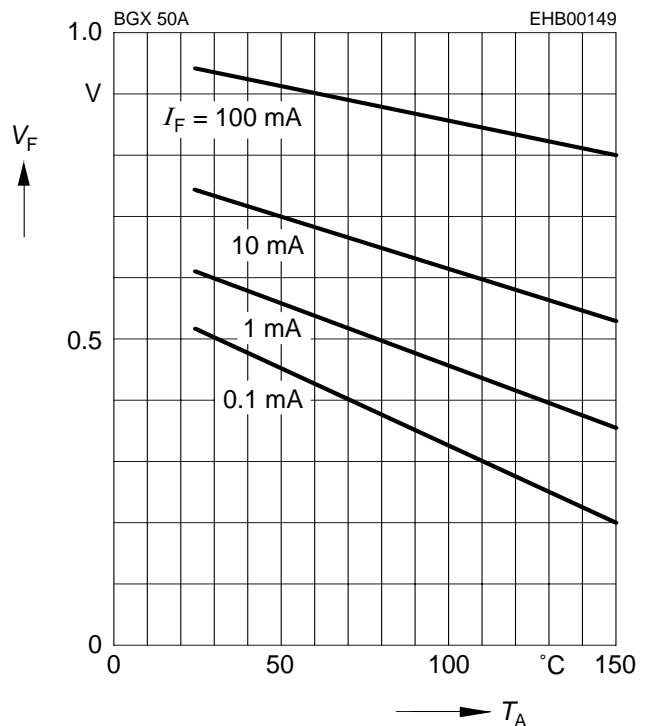


Forward current $I_F = f(V_F)$

$T_A = 25^\circ\text{C}$

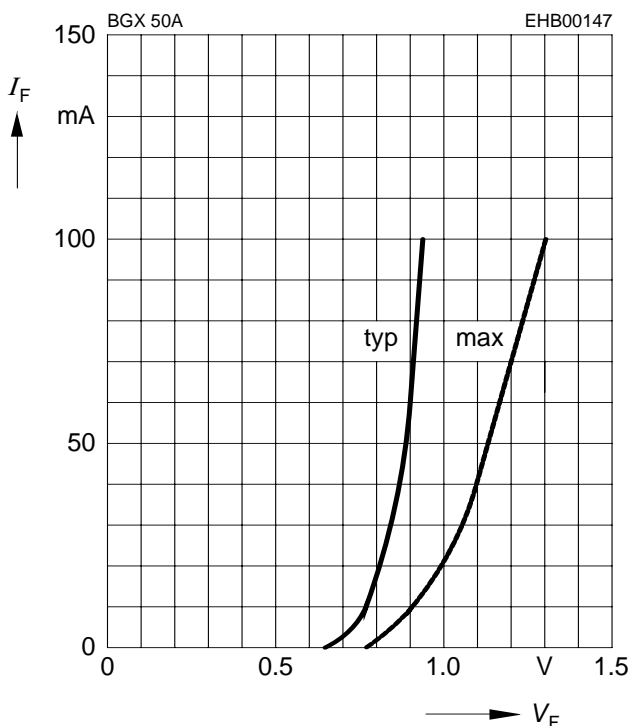

Peak forward current $I_{FM} = f(t_p)$

$T_A = 25^\circ\text{C}$

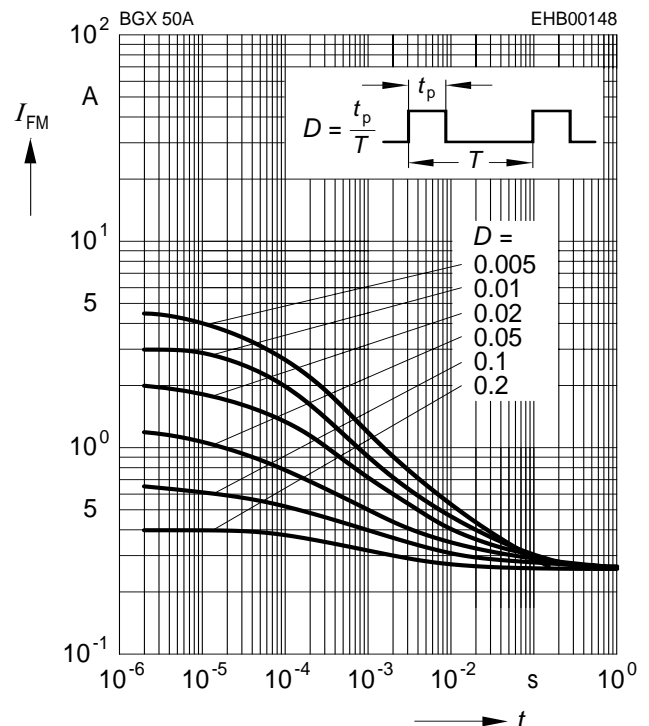




BGX50A...

Forward current $I_F = f(T_S)$

BGX50A

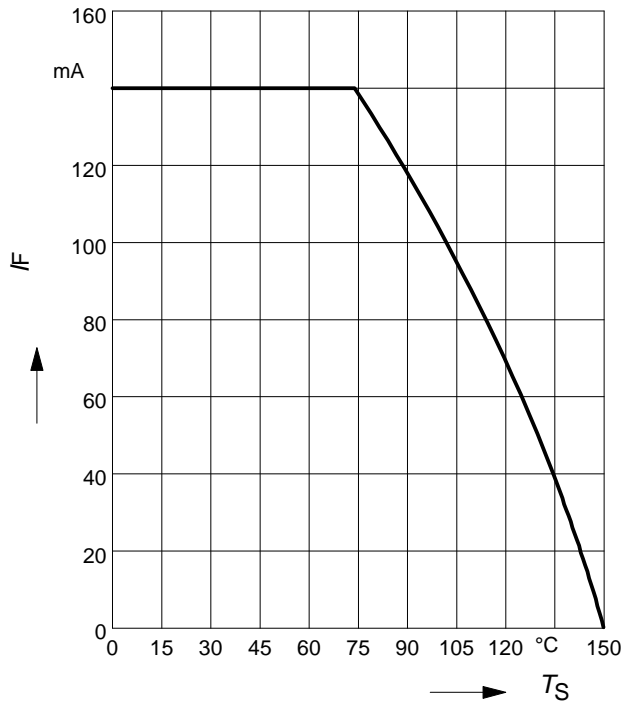





Package SOT143

BGX50A...


Package Outline

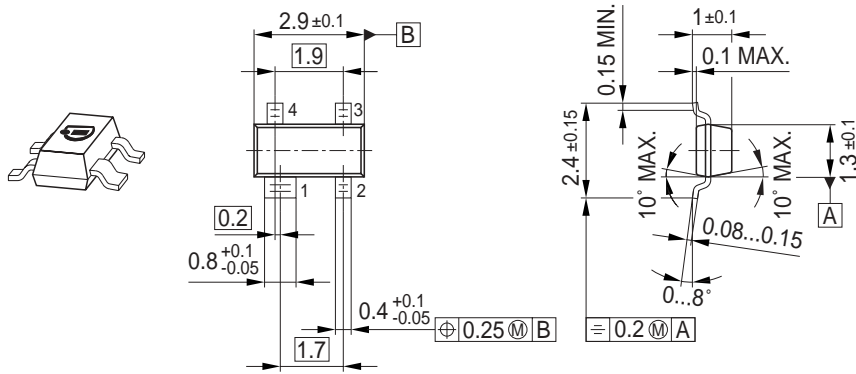

Foot Print




Marking Layout (Example)

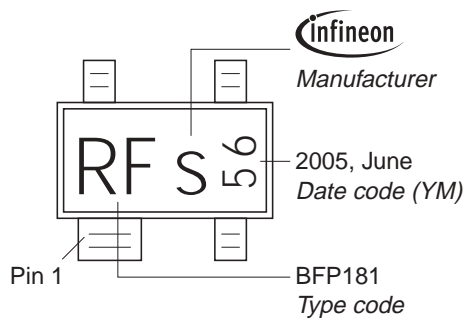

Standard Packing

Reel ø180 mm = 3.000 Pieces/Reel
 Reel ø330 mm = 10.000 Pieces/Reel

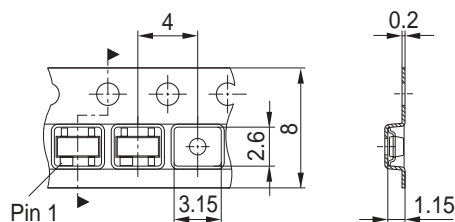



BGX50A...

Edition 2006-02-01

Published by

Infineon Technologies AG

81726 München, Germany

© Infineon Technologies AG 2007.

All Rights Reserved.

Attention please!

The information given in this dokument shall in no event be regarded as a guarantee of conditions or characteristics (“Beschaffenheitsgarantie”). With respect to any examples or hints given herein, any typical values stated herein and/or any information regarding the application of the device, Infineon Technologies hereby disclaims any and all warranties and liabilities of any kind, including without limitation warranties of non-infringement of intellectual property rights of any third party.

Information

For further information on technology, delivery terms and conditions and prices please contact your nearest Infineon Technologies Office (www.infineon.com).

Warnings

Due to technical requirements components may contain dangerous substances. For information on the types in question please contact your nearest Infineon Technologies Office.

Infineon Technologies Components may only be used in life-support devices or systems with the express written approval of Infineon Technologies, if a failure of such components can reasonably be expected to cause the failure of that life-support device or system, or to affect the safety or effectiveness of that device or system.

Life support devices or systems are intended to be implanted in the human body, or to support and/or maintain and sustain and/or protect human life. If they fail, it is reasonable to assume that the health of the user or other persons may be endangered.